

Scanning SQUID susceptometers with sub-micron spatial resolution

John R. Kirtley¹, Lisa Paulius², Aaron J Rosenberg¹, Johanna C. Palmstrom¹, Connor M. Holland¹, Eric M. Spanton¹, Daniel Schiessl³, Colin L. Jermain⁴, Jonathan Gibbons⁴, Y.-K.-K. Fung⁵, Martin E. Huber⁶, Daniel C. Ralph⁷, Mark B Ketchen⁸, Gerald W. Gibson, Jr.⁵, Kathryn A. Moler¹

¹Dept. of Applied Physics - Stanford University - Stanford, CA - USA,

²Dept. of Physics - Western Michigan University - Kalamazoo, MI - USA,

³Attocube Systems AG - Königstraße 11a 80539 - Munich - Germany,

⁴Dept. of Physics - Cornell University - Ithaca, NY - USA,

⁵IBM Research Division - T.J. Watson Research Center - Yorktown Heights, NY - USA,

⁶Dept.'s of Physics and Electrical Engineering - University of Colorado, Denver - Denver, CO - USA,

⁷Dept. of Physics and Kavli Institute at Cornell - Cornell University - Ithaca, NY - USA,

⁸Octevue - Hadley, MA - USA

Email: jkirtley@stanford.edu

October 8, 2016 (STH44, HP117). Scanning SQUID microscopy images local magnetic fields above a sample with excellent sensitivity but modest spatial resolution. A collaborative effort between Stanford University and IBM Research [1] has developed scanning SQUID susceptometers with demonstrated sub-micron spatial resolution [2]. The SQUIDs were fabricated using a Nb/AlO_x/Nb trilayer technology with two additional levels of Nb metal. They include integrated modulation coils for flux feedback, a gradiometric design for insensitivity to uniform magnetic fields, pickup loops for localized flux sensitivity integrated into the body of the SQUID through well-shielded coaxial superconducting lines, and integrated single turn field coils concentric and coaxial with the pickup loops for scanning susceptibility measurements. High spatial resolution is achieved by deep sub-micron lithography, planarization of all levels of metal but the last, and a deep etch step so that the pickup loop can be brought to within a few tenths of a micron from the sample surface, without additional processing of the devices.

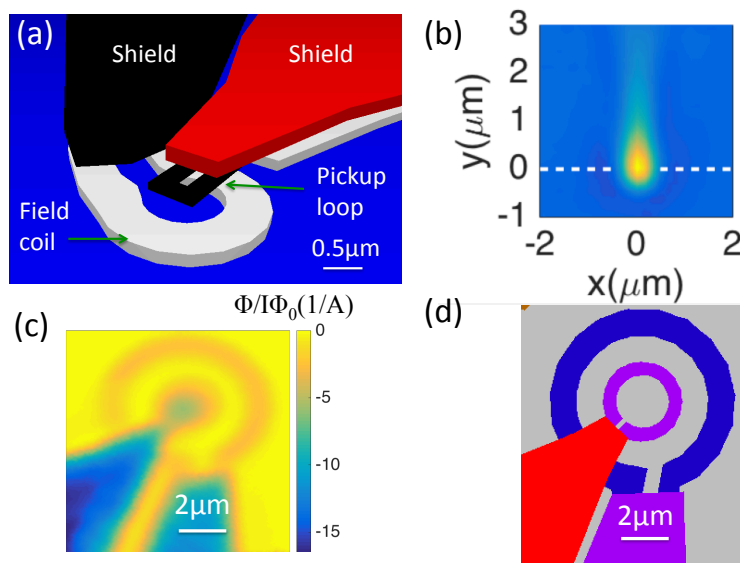


Fig. 1. (a) 3-d rendering of the pickup-loop/field coil region of a 0.2 μm inside diameter pickup loop susceptometer. (b) Magnetometry image of a magnetic nanoparticle. The full-width at half-maximum of a cross-section along the white dashed line is 0.7 μm. (c) Susceptibility image of the pickup-loop/field coil region of a 2 μm inside diameter susceptometer, taken with a 0.2 μm inside diameter pickup loop susceptometer. (d) Layout of the susceptometer imaged in (c).

The paper describes the design, fabrication, and testing of these susceptometers. It also includes modeling and testing of the response of the pickup loop/field coil region to various magnetic field sources, such as magnetic nanoparticles, superconducting vortices, and lines of current. Such modeling is necessary because the characteristic sizes and spacings are comparable to the London penetration depth. This modeling follows closely a prescription given by Brandt [3].

References

- [1] J.R. Kirtley, G.W. Gibson, Jr., Y.-K.-K. Fung, B. Klopfer, K. Nowack, P.A. Kratz, J.-M. Mol, J. Arpes, F. Forooghi, M.E. Huber, H. Bluhm and K.A. Moler, Advanced sensors for scanning SQUID microscopy, *Superconductive Electronics Conference (ISEC), 2013 IEEE 14th International*, 1 (2013).
- [2] John R. Kirtley, Lisa Paulius, Aaron J. Rosenberg, Johanna C. Palmstrom, Connor M. Holland, Eric M. Spanton, Daniel Schiessl, Colin L. Jermain, Jonathan Gibbons, Y.-K.-K. Fung, Martin E. Huber, Daniel C. Ralph, Mark B. Ketchen, Gerald W. Gibson Jr., and Kathryn A. Moler, Scanning SQUID susceptometers with sub-micron spatial resolution, *Rev. Sci. Instr.* **87**, 093702 (2016).
- [3] Ernst Helmut Brandt, Thin superconductors and SQUIDs in perpendicular magnetic field, *Phys. Rev. B* **72**, 024529 (2005).